

---

# PXle-4137

# Specifications

---

2025-09-24



# Contents

PXIe-4137 Specifications ..... 3

# PXIe-4137 Specifications

## PXIe-4137 Specifications

These specifications apply to the PXIe-4137.



**Note** In this document, the PXIe-4137 (40W) and PXIe-4137 (20W) are referred to inclusively as the PXIe-4137. The information in this document applies to all versions of the PXIe-4137 unless otherwise specified. To determine which version of the module you have, locate the device name in one of the following places:

- **In MAX**—The PXIe-4137 (40W) shows **NI PXIe-4137 (40W)**, and the PXIe-4137 (20W) shows as **NI PXIe-4137**.
- **Device front panel**—The PXIe-4137 (40W) shows **PXIe-4137 40W System SMU**, and the PXIe-4137 (20W) shows **NI PXIe-4137 Precision System SMU** on the front panel.

## Definitions

**Warranted** specifications describe the performance of a model under stated operating conditions and are covered by the model warranty.

**Characteristics** describe values that are relevant to the use of the model under stated operating conditions but are not covered by the model warranty.

- **Typical** specifications describe the performance met by a majority of models.
- **Nominal** specifications describe an attribute that is based on design, conformance testing, or supplemental testing.
- **Measured** specifications describe the measured performance of a representative model.

Specifications are **Warranted** unless otherwise noted.

## Conditions

Specifications are valid under the following conditions unless otherwise noted.

- Ambient temperature<sup>1</sup> of  $23\text{ °C} \pm 5\text{ °C}$
- Chassis with slot cooling capacity  $\geq 38\text{ W}^2$ 
  - For chassis with slot cooling capacity = 38 W, fan speed set to HIGH
- Calibration interval of 1 year
- 30 minutes warm-up time
- Self-calibration performed within the last 24 hours
- NI-DCPower Aperture Time is set to 2 power-line cycles (PLC)

## Cleaning Statement



**Notice** Clean the hardware with a soft, nonmetallic brush. Make sure that the hardware is completely dry and free from contaminants before returning it to service.

## PXIe-4137 Pinout

The following figure shows the terminals on the PXIe-4137 connector.

1. The ambient temperature of a PXI system is defined as the temperature at the chassis fan inlet (air intake).
2. For increased capability, NI recommends installing the PXIe-4137 (40W) in a chassis with slot cooling capacity  $\geq 58\text{ W}$ .

Figure 1. PXle-4137 Connector Pinout




Table 1. Signal Descriptions

Signal Name	Description
Output LO	LO force terminal connected to channel power stage (generates and/or dissipates power). Positive polarity is defined as voltage measured on HI > LO.
Sense LO	Voltage remote sense input terminals. Used to compensate for $I \cdot R$ voltage drops in cable leads, connectors, and switches.
Guard	Buffered output that follows the voltage of the HI force terminal. Used to drive shield conductors surrounding HI force and Sense HI conductors to minimize effects of leakage and capacitance on low level currents.
Output HI	HI force terminal connected to channel power stage (generates and/or dissipates power). Positive polarity is defined as voltage measured on HI > LO.
Sense HI	Voltage remote sense input terminals. Used to compensate for $I \cdot R$ voltage drops in cable leads, connectors, and switches.

## Device Capabilities

The following table and figure illustrate the voltage and the current source and sink ranges of the PXIe-4137.


Table 2. Current Source and Sink Ranges

DC voltage ranges	DC current source and sink ranges
600 mV	1 $\mu$ A
6 V	10 $\mu$ A
20 V	100 $\mu$ A
200 V <sup>3</sup>	1 mA
	10 mA
	100 mA
	1 A
	3 A <sup>4</sup>

3. Voltage levels and limits  $>|40 \text{ VDC}|$  require the safety interlock input to be closed.


4. Current is limited to 1 A DC. Higher levels are pulsing only.

Figure 2. Quadrant Diagram for PXIe-4137 (40W)



For additional information related to the Pulse Voltage or Pulse Current settings of the Output Function, for the PXIe-4137 (40W), including pulse on time and duty cycle limits for a particular operating point, refer to [Pulsed Operation](#). For supplementary examples, refer to [Examples of Determining Extended Range Pulse Parameters and Optimizing Slew Rate using NI SourceAdapt](#).

Figure 3. Quadrant Diagram for PXIe-4137 (20W)



DC sourcing power and sinking power are limited to the values in the following table, regardless of output voltage.<sup>5</sup>

Table 3. DC Sourcing & Sinking Power

Model Variant	Chassis Type	DC Sourcing Power	DC Sinking Power
PXIe-4137 (40W)	≥58 W Slot Cooling Capacity	40 W	40 W
	<58 W Slot Cooling Capacity	20 W	12 W
PXIe-4137 (20W)	≥58 W Slot Cooling Capacity	20 W	12 W
	<58 W Slot Cooling Capacity	20 W	12 W



**Caution** Limit DC power sinking to 12 W where applicable as indicated in the above table. For <58 W cooling slots,

5. Power limit defined by voltage measured between HI and LO terminals.

- Additional derating applies to sinking power when operating at an ambient temperature of >45 °C.
- If the PXI Express chassis has multiple fan speed settings, set the fans to the highest setting.

#### Related reference:

- [Sinking Power vs. Ambient Temperature Derating](#)
- [Extended Range Pulsing for PXIe-4137 \(40W\)](#)
- [Extended Range Pulsing for PXIe-4137 \(20W\)](#)

## Voltage

Table 4. Voltage Programming and Measurement Accuracy/Resolution

Range	Resolution (noise limited)	Noise (0.1 Hz to 10 Hz, peak to peak), Typical	Accuracy (23 °C ±5 °C) ± (% of voltage + offset) <sup>6</sup>		Tempco ± (% of voltage + offset)/°C, 0 °C to 55 °C
			T <sub>cal</sub> ±5 °C <sup>[7]</sup> 7	T <sub>cal</sub> ±1 °C <sup>[7]</sup>	
600 mV	100 nV	2 μV	0.020% + 50 μV	0.017% + 30 μV	0.0005% + 1 μV
6 V	1 μV	6 μV	0.020% + 320 μV	0.017% + 90 μV	
20 V	10 μV	20 μV	0.022% + 1 mV	0.017% + 400 μV	
200 V	100 μV	200 μV	0.025% + 10 mV	0.020% + 2.5 mV	

#### Related reference:

- [Noise](#)
- [Load Regulation](#)
- [Remote Sense](#)

6. Accuracy is specified for no load output configurations. Refer to **Load Regulation** and **Remote Sense** sections for additional accuracy derating and conditions.

7. T<sub>cal</sub> is the internal device temperature recorded by the PXIe-4137 at the completion of the last self-calibration.

# Current

Table 5. Current Programming and Measurement Accuracy/Resolution

Range	Resolution (noise limited)	Noise (0.1 Hz to 10 Hz, peak to peak), Typical	Accuracy (23 °C ± 5 °C) ± (% of current + offset)		Tempco ± (% of current + offset)/°C, 0 °C to 55 °C
			T <sub>cal</sub> ± 5 °C [8]	T <sub>cal</sub> ± 1 °C [8]	
1 µA	100 fA	4 pA	0.03% + 100 pA	0.022% + 40 pA	0.0006% + 4 pA
10 µA	1 pA	30 pA	0.03% + 700 pA	0.022% + 300 pA	0.0006% + 22 pA
100 µA	10 pA	200 pA	0.03% + 6 nA	0.022% + 2 nA	0.0006% + 200 pA
1 mA	100 pA	2 nA	0.03% + 60 nA	0.022% + 20 nA	0.0006% + 2 nA
10 mA	1 nA	20 nA	0.03% + 600 nA	0.022% + 200 nA	0.0006% + 20 nA
100 mA	10 nA	200 nA	0.03% + 6 µA	0.022% + 2 µA	0.0006% + 200 nA
1 A	100 nA	2 µA	0.04% + 60 µA	0.035% + 20 µA	0.0006% + 2 µA
3 A <sup>9</sup>	1 µA	20 µA	0.08% + 900 µA	0.075% + 600 µA	0.0018% + 20 µA

## Noise


Wideband source noise	<20 mV peak-to-peak in 20 V range, device configured for normal transient response, 10 Hz to 20 MHz, typical
-----------------------	--------------------------------------------------------------------------------------------------------------

The following figures illustrate measurement noise as a function of measurement

8. T<sub>cal</sub> is the internal device temperature recorded by the PXle-4137 at the completion of the last self-calibration.
9. 3 A range above 1 A is for pulsing only.

aperture for the PXIe-4137.

Figure 4. Voltage Measurement Noise vs. Measurement Aperture, Nominal





 **Note** When the aperture time is set to 2 power-line cycles (PLCs), measurement noise differs slightly depending on whether the Power Line Frequency is set to 50 Hz or 60 Hz.

Figure 5. Current Measurement Noise vs. Measurement Aperture, Nominal





**Note** When the aperture time is set to 2 power-line cycles (PLCs), measurement noise differs slightly depending on whether the Power Line Frequency is set to 50 Hz or 60 Hz.

Related reference:


- [Voltage](#)

## Sinking Power vs. Ambient Temperature Derating

The following figure illustrates sinking power derating as a function of ambient temperature.

This applies to the PXIe-4137 (20W) when used with any chassis and only applies to the PXIe-4137 (40W) when used with a chassis with slot cooling capacity <58 W.

Figure 6. Sinking Power vs. Ambient Temperature Derating



**Note** When using the PXIe-4137 (40W) with a chassis with slot cooling capacity  $\geq 58$  W, ambient temperature derating does not apply.

Related reference:

- [Device Capabilities](#)

## Output Resistance Programming Accuracy

Table 6. Output Resistance Programming Accuracy Characteristics

Current Level/ Limit Range	Programmable Resistance Range, Voltage Mode	Programmable Resistance Range, Current Mode	Accuracy $\pm$ (% of resistance setting), $T_{cal} \pm 5^\circ\text{C}$ <sup>10</sup>
1 $\mu\text{A}$	0 to $\pm 5\text{ M}\Omega$	$\pm 5\text{ M}\Omega$ to $\pm\text{infinity}$	0.03%
10 $\mu\text{A}$	0 to $\pm 500\text{ k}\Omega$	$\pm 500\text{ k}\Omega$ to $\pm\text{infinity}$	
100 $\mu\text{A}$	0 to $\pm 50\text{ k}\Omega$	$\pm 50\text{ k}\Omega$ to $\pm\text{infinity}$	
1 mA	0 to $\pm 5\text{ k}\Omega$	$\pm 5\text{ k}\Omega$ to $\pm\text{infinity}$	
10 mA	0 to $\pm 500\ \Omega$	$\pm 500\ \Omega$ to $\pm\text{infinity}$	
100 mA	0 to $\pm 50\ \Omega$	$\pm 50\ \Omega$ to $\pm\text{infinity}$	
1 A	0 to $\pm 5\ \Omega$	$\pm 5\ \Omega$ to $\pm\text{infinity}$	
3 A <sup>11</sup>	0 to $\pm 500\text{ m}\Omega$	$\pm 500\text{ m}\Omega$ to $\pm\text{infinity}$	

## Overvoltage Protection

Accuracy <sup>12</sup> (% of OVP limit + offset)	0.1% + 200 mV, typical
Temperature coefficient (% of OVP limit + offset)/ $^\circ\text{C}$	0.01% + 3 mV/ $^\circ\text{C}$ , typical
Measurement location	Local sense
Maximum OVP limit value	210 V

10.  $T_{cal}$  is the internal device temperature recorded by the PXIe-4137 at the completion of the last self-calibration.
11. 3 A range above 1 A is for pulsing only.
12. Overvoltage protection accuracy is valid with an ambient temperature of  $23^\circ\text{C} \pm 5^\circ\text{C}$  and with  $T_{cal} \pm 5^\circ\text{C}$ .  $T_{cal}$  is the internal device temperature recorded by the PXIe-4137 at the completion of the last self-calibration.


Minimum OVP limit value	2 V
-------------------------	-----

## Pulsed Operation

Dynamic load, minimum pulse cycle time <sup>13</sup>	100 $\mu\text{s}/\text{A}$
------------------------------------------------------	----------------------------

The following figure visually explains the terms used in the extended range pulsing sections.

Figure 7. Definition of Pulsing Terminology

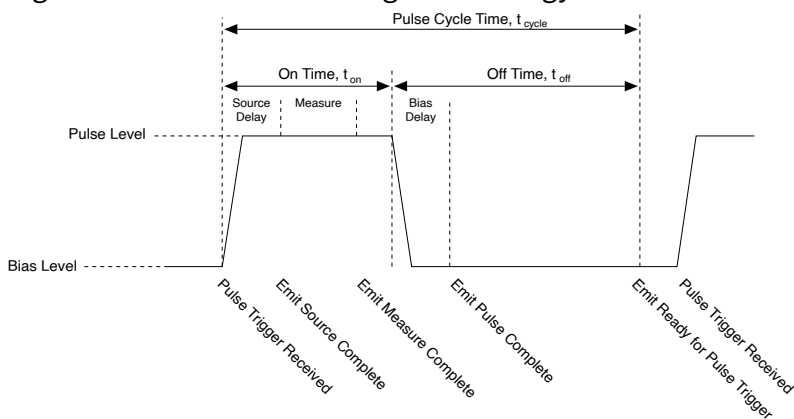

## Extended Range Pulsing for PXIe-4137 (40W)




**Note** Extended range pulses fall outside DC range limits for either current or power. In-range pulses fall within DC range limits and are not subject to extended range pulsing limitations. Extended range pulsing is enabled by setting the Output Function to Pulse Voltage or Pulse Current.

The following figures illustrate the maximum pulse on time and duty cycle for the

- For example, given a continuous pulsing load, if the largest dynamic step in current that the load sources/sinks is from 0.5 A to 1.0 A, then the maximum SMU current step is 0.5 A. Thus, the minimum dynamic load pulse cycle time is 50  $\mu\text{s}$ . Minimum dynamic load pulse cycle time is independent of output voltage.<sup>14</sup>
- Measurable unit of  $\mu\text{s}/\text{A}$  is used because the minimum pulse cycle time is independent of output voltage

PXIe-4137 (40W) in a  $\geq 58$  W cooling slot, for a desired pulse voltage and pulse current given zero bias voltage and current. The shaded areas allow for a quick approximation of output limitations and limiting parameters. Actual limits are described by equations in [Table 7. PXIe-4137 \(40W\) Pulse Level Limits](#).

Figure 8. Pulse On-time vs Pulse Current and Pulse Voltage





 **Note** Equations to solve for maximum pulse on time,  $t_{onMax}$ , are shown in [Table 7. PXIe-4137 \(40W\) Pulse Level Limits](#). Additionally, Equation 8 solves for pulse on time,  $t_{on}$ , in terms of maximum pulse energy in [Example 1: Determining Extended Range Pulse On Time and Duty Cycle Parameters for the \(40W\)](#).

Figure 9. Duty Cycle vs Pulse Current and Pulse Voltage





**Note** Equations to solve for maximum duty cycle,  $D_{Max}$ , are shown in [Table 7. PXle-4137 \(40W\) Pulse Level Limits](#). Additionally, Equation 9 solves for pulse off time,  $t_{off}$ , in terms of maximum pulse energy in [Example 1: Determining Extended Range Pulse On Time and Duty Cycle Parameters for the \(40W\)](#).

Bias level limits	
Maximum voltage, $V_{bias}$	200 V
Maximum current, $I_{bias}$	1 A

Table 7. PXle-4137 (40W) Pulse Level Limits

Specification		Value	Equation
Maximum voltage, $V_{pulseMax}$		160 V	—
Maximum current, $I_{pulseMax}$		3 A	—
Maximum on time, $t_{onMax}$ <sup>15</sup>	If $I_{pulse} > 1$ A and $\geq 58$ W Slot Cooling Capacity Chassis	Calculate using the equation or refer to <a href="#">Figure 8. Pulse On-time vs Pulse Current and Pulse Voltage</a> to estimate the value.	$t_{onMax} = 100 \text{ ms} * \frac{2 \text{ A}}{ I_{pulse}  - 1 \text{ A}}$ , where $t_{onMax}$ is $\leq 167$ s <b>(Equation 1)</b>
	If $I_{pulse} > 1$ A and $< 58$ W Slot Cooling Capacity Chassis	Calculate using the equation.	$t_{onMax} = 10 \text{ ms} * \frac{2 \text{ A}}{ I_{pulse}  - 1 \text{ A}}$ , where $t_{onMax}$ is $\leq 167$ s <b>(Equation 2)</b>
	If $I_{pulse} \leq 1$ A	$t_{onMax} = 167$ s	—
Maximum pulse energy, $E_{pulseMax}$ <sup>16</sup>		0.4 J	—

15. **Pulse on time** is measured from the start of the leading edge to the start of the trailing edge. See [Figure 7. Definition of Pulsing Terminology](#).

Specification		Value	Equation
			$E_{\text{pulse}} =  V_{\text{pulse}} * I_{\text{pulse}} * t_{\text{on}} $ , where $E_{\text{pulse}} < E_{\text{pulseMax}}$ <b>(Equation 3)</b>
Maximum duty cycle, $D_{\text{Max}}$ <sup>17</sup>	If $\geq 58$ W Slot Cooling Capacity Chassis	Calculate using the equation or refer to <a href="#">Figure 9. Duty Cycle vs Pulse Current and Pulse Voltage</a> to estimate the value.	$D_{\text{Max}} = \frac{(1.18 \text{ A})^2 -  I_{\text{bias}} ^2}{ I_{\text{pulse}} ^2 -  I_{\text{bias}} ^2} * 100\%$ <b>(Equation 4)</b>
	If $< 58$ W Slot Cooling Capacity Chassis	Calculate using the equation.	$D_{\text{Max}} = \frac{(1 \text{ A})^2 -  I_{\text{bias}} ^2}{ I_{\text{pulse}} ^2 -  I_{\text{bias}} ^2} * 100\%$ <b>(Equation 5)</b>
Minimum pulse cycle time, $t_{\text{cycleMin}}$		5 ms	$t_{\text{cycle}} = t_{\text{on}} + t_{\text{off}}$ , where $t_{\text{cycle}} > t_{\text{cycleMin}}$ <b>(Equation 6)</b>
Maximum cycle average power, $P_{\text{CAMax}}$ <sup>18</sup>	$\geq 58$ W Slot Cooling Capacity Chassis	20 W	$P_{\text{CA}} = \frac{ V_{\text{pulse}} * I_{\text{pulse}} * t_{\text{on}}  +  V_{\text{bias}} * I_{\text{bias}} * t_{\text{off}} }{t_{\text{on}} + t_{\text{off}}}$ , where $P_{\text{CA}} < P_{\text{CAMax}}$ <b>(Equation 7)</b>
	$< 58$ W Slot Cooling Capacity Chassis	10 W	

16. Refer to [Figure 8. Pulse On-time vs Pulse Current and Pulse Voltage](#) to estimate the value and determine the limiting equation for a PXIe-4137 (40W) in a  $\geq 58$  W Slot Cooling Capacity Chassis.
17. Refer to [Figure 9. Duty Cycle vs Pulse Current and Pulse Voltage](#) to estimate the value and determine the limiting equation for a PXIe-4137 (40W) in a  $\geq 58$  W Slot Cooling Capacity Chassis. If  $D \geq 100\%$ , consider switching Output Function from Pulse mode to DC mode.
18. Refer to [Figure 9. Duty Cycle vs Pulse Current and Pulse Voltage](#) to estimate the value and determine the limiting equation for a PXIe-4137 (40W) in a  $\geq 58$  W Slot Cooling Capacity Chassis.



**Note** Software will not allow settings that violate these limiting equations and will generate an error.

#### Related reference:

- [Device Capabilities](#)

## Extended Range Pulsing for PXle-4137 (20W)



**Note** Extended range pulses fall outside DC range limits for either current or power. In-range pulses fall within DC range limits and are not subject to extended range pulsing limitations. Extended range pulsing is enabled by configuring the Output Function to Pulse Voltage or Pulse Current.

Bias level limits	
Maximum voltage	200 V
Maximum current	1 A
Pulse level limits	
Maximum voltage	160 V
Maximum current	3 A
Maximum on time <sup>19</sup>	1 ms
Minimum pulse cycle time	5 ms
Energy	0.2 J

Maximum cycle average power	10 W
Maximum duty cycle	5%

### Related reference:

- [Device Capabilities](#)

## Transient Response and Settling Time

Transient response	<70 $\mu\text{s}$ to recover within 0.1% of voltage range after a load current change from 10% to 90% of range, device configured for fast transient response, typical	
Maximum slew rate <sup>20,21</sup>	0.5A/ $\mu\text{s}$	
<b>Settling time</b> <sup>22</sup>		
Voltage mode, 180 V step, unloaded <sup>23</sup>		<500 $\mu\text{s}$ , typical
Voltage mode, 5 V step or smaller, unloaded <sup>24</sup>		<70 $\mu\text{s}$ , typical
Current mode, full-scale step, 3 A to 100 $\mu\text{A}$ ranges <sup>25[25]</sup>		<50 $\mu\text{s}$ , typical

19. **Pulse on time** is measured from the start of the leading edge to the start of the trailing edge. See [Figure 7. Definition of Pulsing Terminology](#).
20. Optimize transient response, overshoot, and slew rate with NI SourceAdapt by adjusting the Transient Response.
21. To improve the slew rate, see [Examples of Determining Extended Range Pulse Parameters and Optimizing Slew Rate using NI SourceAdapt](#).
22. Measured as the time to settle to within 0.1% of step amplitude, device configured for fast transient

Current mode, full-scale step, 10 $\mu\text{A}$ range <sup>[25]</sup>	<150 $\mu\text{s}$ , typical
Current mode, full-scale step, 1 $\mu\text{A}$ range <sup>[25]</sup>	<300 $\mu\text{s}$ , typical

The following figures illustrate the effect of the transient response setting on the step response of the PXIe-4137 for different loads.

Figure 10. 1 mA Range, No Load Step Response, Nominal





Figure 11. 1 mA Range, 100 nF Load Step Response, Nominal



## Load Regulation

### Voltage

response.

23. Current limit set to  $\geq 60 \mu\text{A}$  and  $\geq 60\%$  of the selected current limit range.
24. Current limit set to  $\geq 20 \mu\text{A}$  and  $\geq 20\%$  of selected current limit range.
25. Voltage limit set to  $\geq 2 \text{ V}$ , resistive load set to  $1 \text{ V}/\text{selected current range}$ .

Device configured for local sense	200 mV per A of output load change (measured between output channel terminals), typical
Device configured for remote sense	100 $\mu$ V per A of output load change (measured between sense terminals), typical

Current, device configured for local or remote sense	Load regulation effect included in current accuracy specifications, typical
------------------------------------------------------	-----------------------------------------------------------------------------

### Related reference:

- [Voltage](#)

## Expected Relay Life

Output Connected	$\geq 100$ k cycles
------------------	---------------------



**Note** To avoid excessive relay wear, do not set Output Connected to **TRUE** when a non-zero voltage is connected to the output.

## Measurement and Update Timing Characteristics

Available sample rates <sup>26</sup>	$(1.8 \text{ MS/s})/N$ where $N = 1, 2, 3, \dots 2^{24}$ , nominal
Sample rate accuracy	Equal to PXIe_CLK100 accuracy, nominal

26. When sourcing while measuring, both the Source Delay and Aperture Time affect the sampling rate. When taking a measure record, only the Aperture Time affects the sampling rate.

Maximum measure rate to host	1.8 MS/s per channel, continuous, nominal	
<b>Maximum source update rate<sup>27</sup></b>		
Sequence mode	100,000 updates/s (10 $\mu$ s/update), nominal	
Timed output mode	80,000 updates/s (12.5 $\mu$ s/update), nominal	
<b>Input trigger to</b>		
Source event delay	10 $\mu$ s, nominal	
Source event jitter	1 $\mu$ s, nominal	
Measure event jitter	1 $\mu$ s, nominal	
<b>Pulse mode timing and accuracy<sup>28</sup></b>		
<b>Minimum pulse on time<sup>29</sup></b>		
PXIe-4137 (40W) <sup>30</sup>	10 $\mu$ s, nominal	
PXIe-4137 (20W)	50 $\mu$ s, nominal	
Minimum pulse off time <sup>31</sup>	50 $\mu$ s, nominal	
Pulse on time or off time programming resolution	100 ns, nominal	

27. As the source delay is adjusted or if advanced sequencing is used, maximum source rates vary. Timed output mode is enabled in Sequence Mode by setting Sequence Step Delta Time Enabled to True. Additional timing limitations apply when operating in pulse mode (Output Function is set to Pulse Voltage or Pulse Current).

Pulse on time or off time programming accuracy	$\pm 5 \mu\text{s}$ , nominal
Pulse on time or off time jitter	1 $\mu\text{s}$ , nominal

## Remote Sense

Voltage accuracy	Add 3 ppm of voltage range per volt of HI lead drop plus 1 $\mu\text{V}$ per volt of lead drop per ohm of corresponding sense lead resistance to voltage accuracy specifications
Maximum sense lead resistance	100 $\Omega$
Maximum lead drop per lead	3 V, maximum 202 V between HI and LO terminals



**Note** Exceeding the maximum lead drop per lead value may cause the driver to report a sense lead error.

### Related reference:

- [Voltage](#)

- Pulse mode is enabled when the Output Function is set to Pulse Voltage or Pulse Current. This mode enables access to extended range pulsing capabilities. For PXIe-4137 (20W), shorter minimum on times for in-range pulses can be achieved using Sequence mode or Timed Output mode with the Output Function set to Voltage or Current.
- Pulse on time** is measured from the start of the leading edge to the start of the trailing edge. See [Figure 7. Definition of Pulsing Terminology](#).
- Optimize transient response, overshoot, and slew rate with NI SourceAdapt by adjusting the Transient Response.
- Pulses fall inside DC limits. **Pulse off time** is measured from the start of the trailing edge to the start of a subsequent leading edge.

## Safety Interlock

The safety interlock feature is designed to prevent users from coming in contact with hazardous voltage generated by the SMU in systems that implement protective barriers with controlled user access points.



**Caution** Hazardous voltages of up to the maximum voltage of the PXIe-4137 may appear at the output terminals if the safety interlock terminal is closed. Open the safety interlock terminal when the output connections are accessible. With the safety interlock terminal open, the output voltage level/limit is limited to  $\pm 40$  V DC, and protection will be triggered if the voltage measured between the device HI and LO terminals exceeds  $\pm(42$  V peak  $\pm 0.4$  V).



**Attention** Des tensions dangereuses allant jusqu'à la tension maximale du PXIe-4137 peuvent apparaître aux terminaux de sortie si le terminal de verrouillage de sécurité est fermé. Ouvrez le terminal de verrouillage de sécurité lorsque les connexions de sortie sont accessibles. Lorsque le terminal de verrouillage de sécurité est ouvert, le niveau ou la limite de tension de sortie est limité à  $\pm 40$  V CC, et la protection se déclenchera si la tension mesurée entre les terminaux HI et LO de l'appareil dépasse  $\pm (42$  Vpic  $\pm 0,4$  V).



**Caution** Do not apply voltage to the safety interlock connector inputs. The interlock connector is designed to accept passive, normally open contact closure connections only.



**Attention** N'appliquez pas de tension aux entrées du connecteur de verrouillage de sécurité. Le connecteur de verrouillage est conçu pour accepter uniquement des connexions à fermeture de contact passives, normalement ouvertes.

Safety interlock terminal open

Output	<±42.4 V peak
Setpoint	<±40 V DC
<b>Safety interlock terminal closed</b>	
Output	Maximum voltage of the device
Setpoint	Maximum selected voltage range

## Examples of Calculating Accuracy Specifications



**Note** Specifications listed in examples are for demonstration purposes only and do not necessarily reflect specifications for this device.

### Example 1: Calculating 5 °C Accuracy

Calculate the accuracy of 900 nA output in the 1 µA range under the following conditions:

Ambient temperature	28 °C
Internal device temperature	within $T_{cal} \pm 5 \text{ °C}$ <sup>32</sup>
Self-calibration	within the last 24 hours

**Solution:** Because the device internal temperature is within  $T_{cal} \pm 5 \text{ °C}$  and the ambient temperature is within  $23 \text{ °C} \pm 5 \text{ °C}$ , the appropriate accuracy specification is the following value:

0.03% + 100 pA

32.  $T_{cal}$  is the internal device temperature recorded by the PXle-4137 at the completion of the last self-calibration.

Calculate the accuracy using the following formula:

$$\begin{aligned} \text{Accuracy} &= 900 \text{ nA} * 0.03 \% + 100\text{pA} \\ &= 270\text{pA} + 100\text{pA} \\ &= 370\text{pA} \end{aligned}$$

Therefore, the actual output is within 370 pA of 900 nA.

## Example 2: Calculating Remote Sense Accuracy

Calculate the remote sense accuracy of 500 mV output in the 600 mV range. Assume the same conditions as in Example 1, with the following differences:

HI path lead drop	3 V
HI sense lead resistance	2 $\Omega$
LO path lead drop	2.5 V
LO sense lead resistance	1.5 $\Omega$

Solution: Because the device internal temperature is within  $T_{\text{cal}} \pm 5 \text{ }^\circ\text{C}$  and the ambient temperature is within  $23 \text{ }^\circ\text{C} \pm 5 \text{ }^\circ\text{C}$ , the appropriate accuracy specification is the following value:

$$0.02\% + 50 \mu\text{V}$$

Because the device is using remote sense, use the following remote sense accuracy specification:

Add 3 ppm of voltage range per volt of HI lead drop plus 1  $\mu\text{V}$  per volt of lead drop per  $\Omega$  of corresponding sense lead resistance to voltage accuracy specifications.

Calculate the remote sense accuracy using the following formula:

$$\begin{aligned} \text{Accuracy} &= \left( 500 \text{ mV} * 0.02 \% + 50 \mu\text{V} \right) + \frac{600 \text{ mV} * 3 \text{ ppm}}{1 \text{ V of lead drop}} * 3 \text{ V} + \frac{1 \mu\text{V}}{\text{V} * \Omega} * 3 \text{ V} * 2 \Omega + \frac{1 \mu\text{V}}{\text{V} * \Omega} * 2.5 \text{ V} * 1.5 \Omega \\ &= 100\mu\text{V} + 50\mu\text{V} + 1.8\mu\text{V} * 3 + 6\mu\text{V} + 3.75\mu\text{V} \\ &= 165.15\mu\text{V} \end{aligned}$$

Therefore, the actual output is within 165.15  $\mu\text{V}$  of 500 mV.

## Example 3: Calculating Accuracy with Temperature Coefficient

Calculate the accuracy of 900 nA output in the 1  $\mu\text{A}$  range. Assume the same conditions as in Example 1, with the following differences:

Ambient temperature	15 $^{\circ}\text{C}$
---------------------	-----------------------

Solution: Because the device internal temperature is within  $T_{\text{cal}} \pm 5^{\circ}\text{C}$ , the appropriate accuracy specification is the following value:

$$0.03\% + 100 \text{ pA}$$

Because the ambient temperature falls outside of  $23^{\circ}\text{C} \pm 5^{\circ}\text{C}$ , use the following temperature coefficient per  $^{\circ}\text{C}$  outside the  $23^{\circ}\text{C} \pm 5^{\circ}\text{C}$  range:

$$0.0006\% + 4 \text{ pA}$$

Calculate the accuracy using the following formula:

$$\text{TemperatureVariation} = (23^{\circ}\text{C} - 5^{\circ}\text{C}) - 15^{\circ}\text{C} = 3^{\circ}\text{C}$$

$$\text{Accuracy} = (900 \text{ nA} * 0.03\% + 100 \text{ pA}) + \frac{900 \text{ nA} * 0.0006\% + 4 \text{ pA}}{1^{\circ}\text{C}} * 3^{\circ}\text{C}$$

$$= 370 \text{ pA} + 28.2 \text{ pA}$$

$$= 398.2 \text{ pA}$$

Therefore, the actual output is within 398.2 pA of 900 nA.

# Examples of Determining Extended Range Pulse Parameters and Optimizing Slew Rate using NI SourceAdapt



**Note** Specifications listed in examples are for demonstration purposes only and do not necessarily reflect specifications for this device.

## Example 1: Determining Extended Range Pulse On Time and Duty Cycle Parameters for the PXIe-4137 (40W)

Determine the extended range pulsing parameters, assuming the following operating point.

Output function	Pulse Current
Pulse voltage limit, $V_{\text{pulse}}$	80 V
Pulse current level, $I_{\text{pulse}}$	3 A
Bias voltage limit, $V_{\text{bias}}$	0.1 V
Bias current level, $I_{\text{bias}}$	0 A
Pulse on time, $t_{\text{on}}$	1.5 ms
Chassis' slot cooling capacity	$\geq 58$ W

### Solution

Begin by calculating the pulse power using the following equation.

$$\begin{aligned}
 \text{Pulse power} &= V_{\text{pulse}} * I_{\text{pulse}} \\
 &= 80 \text{ V} * 3 \text{ A} \\
 &= 240 \text{ W}
 \end{aligned}$$

For PXIe-4137 (40W), refer to the following figures to identify next steps. First, verify the the region of operation using [Figure 1](#), which shows 240 W is in the extended range

pulsing region.

Next, refer to [Figure 8. Pulse On-time vs Pulse Current and Pulse Voltage](#), which shows the maximum pulse on time,  $t_{on}$ , is limited by the maximum pulse energy,  $E_{pulseMax}$ . Use the pulse energy equation (**Equation 3**) from [Table 7. PXIe-4137 \(40W\) Pulse Level Limits](#) to calculate the maximum pulse on time,  $t_{onMax}$  (**Equation 8**).

$$t_{onMax} = \left| \frac{E_{pulseMax}}{V_{pulse} * I_{pulse}} \right| \quad (Eq.8)$$

$$= \left| \frac{0.4 \text{ J}}{80 \text{ V} * 3 \text{ A}} \right|$$

$$= 1.67 \text{ ms}$$

Next, refer to [Figure 9. Duty Cycle vs Pulse Current and Pulse Voltage](#), which shows the maximum duty cycle,  $D$ , is limited by the cycle average power,  $P_{CA}$ . If the required pulse on time is 1.5 ms and the module is installed in a chassis with slot cooling capacity  $\geq 58$  W, use the cycle average power equation (**Equation 7**) from [Table 7. PXIe-4137 \(40W\) Pulse Level Limits](#) to calculate the minimum pulse off time,  $t_{offMin}$  (**Equation 9**).

$$t_{offMin} = \left| \frac{P_{CA} * t_{on} - V_{pulse} * I_{pulse} * t_{on}}{P_{CA} - V_{bias} * I_{bias}} \right| \quad (Eq.9)$$

$$= \left| \frac{20 \text{ W} * 1.5 \text{ ms} - 80 \text{ V} * 3 \text{ A} * 1.5 \text{ ms}}{20 \text{ W} - 0.1 \text{ V} * 0 \text{ A}} \right|$$

$$= 16.5 \text{ ms}$$

Finally, verify that the pulse cycle time,  $t_{cycle}$ , is greater than or equal to the minimum pulse cycle time,  $t_{cycleMin}$  (5 ms). To calculate the pulse cycle time, use the following equation:

$$t_{cycle} = t_{on} + t_{off} \quad (Eq. 6)$$

$$= 1.5 \text{ ms} + 16.5 \text{ ms}$$

$$= 18 \text{ ms}$$

In this case, the pulse cycle time meets the minimum pulse cycle time specification.

Therefore, a 80 V, 3 A pulse with an on time of 1.5 ms and a pulse off time of 16.5 ms is supported, since it fulfills the following criteria:

- Greater than the minimum pulse on time of 10  $\mu\text{s}$
- Equal to the minimum pulse off time of 16.5 ms to meet maximum cycle average power
- Greater than the minimum pulse cycle time of 5 ms

## Example 2: Determining Extended Range Pulse On Time and Duty Cycle Parameters for the PXIe-4137 (20W)

Determine the extended range pulsing parameters, assuming the following operating point.

Output function	Pulse Current
Pulse voltage limit, $V_{\text{pulse}}$	80 V
Pulse current level, $I_{\text{pulse}}$	3 A
Bias voltage limit, $V_{\text{bias}}$	0.1 V
Bias current level, $I_{\text{bias}}$	0 A
Pulse on time, $t_{\text{on}}$	1.5 ms
Chassis' slot cooling capacity	$\geq 58$ W

### Solution

Begin by calculating the pulse power using the following equation.

$$\begin{aligned}
 \text{Pulse power} &= V_{\text{pulse}} * I_{\text{pulse}} \\
 &= 80 \text{ V} * 3 \text{ A} \\
 &= 240 \text{ W}
 \end{aligned}$$

Since the pulse power of 240 W is within the 480 W region of [Figure 3. Quadrant Diagram for PXIe-4137 \(20W\)](#), the maximum configurable on time is 400  $\mu\text{s}$  and maximum duty cycle is 2%.

For example, if the required pulse on time is 100  $\mu\text{s}$ , and the required pulse cycle time

is 10 ms, calculate the pulse off time and verify the duty cycle using the following equations.

$$\begin{aligned} t_{\text{off}} &= t_{\text{cycle}} - t_{\text{on}} \\ &= 10 \text{ ms} - 100 \text{ } \mu\text{s} \\ &= 9.9 \text{ ms} \end{aligned}$$

$$\begin{aligned} \text{Duty cycle} &= \frac{t_{\text{on}}}{t_{\text{cycle}}} * 100\% \\ &= 1 \text{ \%} \end{aligned}$$

Therefore, a pulse with an on time of 100  $\mu\text{s}$  and 1% duty cycle would be supported, since it fulfills the following criteria:

- Greater than the minimum pulse on time of 50  $\mu\text{s}$
- Less than the maximum pulse on time of 400  $\mu\text{s}$  and duty cycle of 2%
- Greater than the minimum pulse cycle time of 5 ms


## Example 3: Using NI SourceAdapt to Increase the Slew Rate of the Pulse

Determine the appropriate operating parameters and custom transient response settings, assuming the following example parameters.

Output function	Pulse Current
Pulse voltage limit, $V_{\text{pulse}}$	160 V
Pulse current level, $I_{\text{pulse}}$	3 A
Bias voltage limit, $V_{\text{bias}}$	0.1 V
Bias current level, $I_{\text{bias}}$	0 A
Transient response	Fast
Load, cable impedance	22.3 $\Omega$ , 1.8 $\mu\text{H}$
Pulse on time, $t_{\text{on}}$	10 $\mu\text{s}$
Pulse off time, $t_{\text{off}}$	4.99 ms

The SMU Transient Response can be configured to three predefined settings, Slow, Normal, and Fast. If these settings do not provide the desired pulse response, a fourth setting, Custom, enables NI SourceAdapt<sup>33</sup> technology which provides the ability to customize the SMU response to any load, and achieve an ideal response with minimum rise times and no overshoots or oscillations.

Figure 12. 10  $\mu$ s Pulse Output with Load, Fast Transient Response




## Solution

SourceAdapt allows users to set the desired gain bandwidth, compensation frequency, and pole-zero ratio through custom transient response to obtain the desired pulse waveform. To use SourceAdapt, first set the Transient Response to Custom.

To achieve the resulting waveform in the following figure, use the parameters in the following table.

33. Visit [ni.com](http://ni.com) for more information about NI SourceAdapt Next-Generation SMU Technology.


Figure 13. 10 μs Pulse Output with Load, Custom Transient Response



Transient response	Custom
Current: Gain bandwidth	900 kHz
Current: Compensation frequency	200 kHz
Current: Pole-zero ratio	2

Gain bandwidth is directly proportional to the step response slew rate. The higher the gain bandwidth, the higher the slew rate. It is worth noting that increasing the gain bandwidth will likely increase ringing. However, this can likely be removed by appropriately setting the compensation frequency and the pole-zero ratio.

Figure 14. Example of Ringing Frequency



Compensation frequency and pole-zero ratio are used to determine the frequencies of the SMU control loop pole and zero, which can be used to optimize the system transient response by increasing phase margin and reducing ringing. To reduce the

overshoot, it is recommended to set the compensation frequency close to the overshoot ringing frequency, see  $F_c$  in the figure above, and set the pole-zero ratio to be greater than 1.

For reference, the pole frequency and zero frequency are derived by the following equations.

$$\text{Pole frequency} = \text{Compensation frequency} * \sqrt{\text{Pole-zero ratio}}$$

$$\text{Zero frequency} = \frac{\text{Compensation frequency}}{\text{Pole-zero ratio}}$$

These settings can be accessed through the Transient Response set to Custom: Voltage or Current.

## Trigger Characteristics

### Input triggers

Types	Start, Source, Sequence Advance, Measure, Pulse	
<b>Sources (PXI trigger lines &lt;0...7&gt;)</b> <sup>34</sup>		
Polarity	Configurable	
Minimum pulse width	100 ns, nominal	
<b>Destinations</b> <sup>35</sup> (PXI trigger lines <0...7>)		
Polarity	Active high (not configurable)	
Pulse width	>200 ns, typical	

34. Pulse widths and logic levels are compliant with ***PXI Express Hardware Specification Revision 1.0 ECN 1***.

35. Input triggers can be re-exported.

## Output triggers (events)

Types	Source Complete, Sequence Iteration Complete, Sequence Engine Done, Measure Complete, Pulse Complete, Ready for Pulse
<b>Destinations (PXI trigger lines &lt;0...7&gt;)</b>	
Polarity	Configurable
Pulse width	Configurable between 250 ns and 1.6 $\mu$ s, nominal

## Protection

<b>Output channel protection</b>	
Overcurrent or overvoltage	Automatic shutdown, output disconnect relay opens
Sink overload protection	Automatic shutdown, output disconnect relay opens
Overtemperature	Automatic shutdown, output disconnect relay opens
Safety interlock	Disable high voltage output, output disconnect relay opens

## Safety Voltage and Current



**Notice** The protection provided by the PXIe-4137 can be impaired if it is used in a manner not described in the user documentation.



**Warning** Take precautions to avoid electrical shock when operating this

product at hazardous voltages.



**Caution** Isolation voltage ratings apply to the voltage measured between any channel pin and the chassis ground. When operating channels in series or floating on top of external voltage references, ensure that no terminal exceeds this rating.



**Attention** Les tensions nominales d'isolation s'appliquent à la tension mesurée entre n'importe quelle broche de voie et la masse du châssis. Lors de l'utilisation de voies en série ou flottantes en plus des références de tension externes, assurez-vous qu'aucun terminal ne dépasse cette valeur nominale.

DC voltage	±200 V
<b>Channel-to-earth ground isolation</b>	
Continuous	250 V DC, CAT I
Withstand	1,000 V RMS, verified by a 5 s withstand



**Caution** Do not connect the PXle-4137 to signals or use for measurements within Measurement Categories II, III, or IV.



**Attention** Ne connectez pas le PXle-4137 à des signaux et ne l'utilisez pas pour effectuer des mesures dans les catégories de mesure II, III ou IV.

Measurement Category I is for measurements performed on circuits not directly connected to the electrical distribution system referred to as **MAINS** voltage. MAINS is a hazardous live electrical supply system that powers equipment. This category is for measurements of voltages from specially protected secondary circuits. Such voltage

measurements include signal levels, special equipment, limited-energy parts of equipment, circuits powered by regulated low-voltage sources, and electronics.



**Note** Measurement Categories CAT I and CAT O are equivalent. These test and measurement circuits are for other circuits not intended for direct connection to the MAINS building installations of Measurement Categories CAT II, CAT III, or CAT IV.

DC current range	$\pm 1$ A; $\pm 3$ A, pulse only
------------------	----------------------------------

## Guard Output Characteristics

Cable guard	
Output impedance	3 k $\Omega$ , nominal
Offset voltage	1 mV, typical

## Calibration Interval

Recommended calibration interval	1 year
----------------------------------	--------

## Power Requirement

PXle-4137 (40W)	3.0 A from the 3.3 V rail and 6.0 A from the 12 V rail
PXle-4137 (20W)	2.5 A from the 3.3 V rail and 2.7 A from the 12 V rail

## Physical

Dimensions	3U, one-slot, PXI Express/CompactPCI Express module 2.0 cm × 13.0 cm × 21.6 cm (0.8 in. × 5.1 in. × 8.5 in.)	
<b>Weight</b>		
PXIe-4137 (20W)	419 g (14.8 oz)	
PXIe-4137 (40W)	428 g (15.1 oz)	
Front panel connectors	5.08 mm (8 position) combicon, 1 × 4.08 mm (3 position) combicon	

## Environmental Characteristics

Table 8. Temperature

Operating	0 °C to 55 °C
Storage	-40 °C to 71 °C

Table 9. Humidity

Operating	10% to 90%, noncondensing
Storage	5% to 95%, noncondensing

Table 10. Pollution Degree

Pollution degree	2
------------------	---

Table 11. Maximum Altitude

Maximum altitude	2,000 m (800 mbar) (at 25 °C ambient temperature)
------------------	---------------------------------------------------

Table 12. Shock and Vibration

Operating vibration	5 Hz to 500 Hz, 0.3 g RMS
Non-operating vibration	5 Hz to 500 Hz, 2.4 g RMS
Operating shock	30 g, half-sine, 11 ms pulse